

tests/box  
**5**



**FPV Ag**  
Vet Expert Rapid Test



**EN** | Rapid test for the qualitative detection of Feline Parvovirus antigen.

**PL** | Szybki test do jakościowego wykrywania antygenu parwowirusa kotów.

**FR** | Test rapide de détection qualitative de l'antigène du Parvovirus félin.

**CZ** | Rychlý test pro kvalitativní detekci antigenu kočičího parvoviru.

**DE** | Schnelltest zum qualitativen Nachweis von Felinem Parvovirus-Antigen.

**UA** | Швидкий тест для якісного виявлення антигену парвовірусу у котів.

**GR** | Ταχία διαγνωστική δοκιμή για την ποιοτική ανίχνευση του αντιγόνου του Πανλευκοϊκού της γάτας.

**ES** | Prueba rápida para la detección cualitativa del antígeno del parvovirus felino. Uso veterinario. Producto de Venta Libre. Manténgase fuera del alcance de los niños. Almacenar a temperatura ambiente o refrigerado, entre 2-30°C. No congelar. Instrucciones completas en el inserto adjunto.

**RO** | Kit testare rapida pentru detectarea calitativa a antigenului Feline Parvovirus.

**TR** | Feline Parvovirus antijenininin kalitatif tespiti için hızlı test.

**PT** | Teste rápido para deteção qualitativa do antígeno do parvovirus felino.

Importado y distribuido por Hallmark S.A. Las Magnolias Mz G1. Lote 5. Lima 15. Perú.  
Elaborado por:  
Vet Planet Sp. z o. o. ul. Brukowa 36/2 05-092 Lomianki, Polonia.

Dodávateľ:  
Vet Planet Czech Republic, s.r.o.,  
Chlumecká 3203,  
198 29 Praha 9 - Černý Most

Представник в Україні:  
ТОВ «Барбус»  
вул. Велика Арнаутська, 17, м.  
Одеса, 65125  
тел./факс: (048) 777 25 71  
e-mail: info@barbus.net

Εισάγεται και διανέμεται:  
Anicel, OE - Α.Δημοκρατίας  
257 - Αγιορείς - Τηλ: 2114110700  
Μ.Ε.Ζ. 02200 025 000060.

Dogerty Grupo Empresarial S.L.  
ES811722642  
PARQUE EMPRESARIAL  
C/ DESARROLLO PARCELA B-8  
Tlfn.: 956 184 490  
Fax.: 956 184 754  
11407 JEREZ DE LA FRONTERA  
CADIZ R-1011



5 902414 201064



Vet Expert Rapid Test  
**FPV Ag**



**5**  
tests/box



feces

Vet Expert Rapid Test  
**FPV Ag**  
For veterinary use only

**IVD** For in vitro diagnostics use only

Store at  
2°C - 30°C

See instructions for use

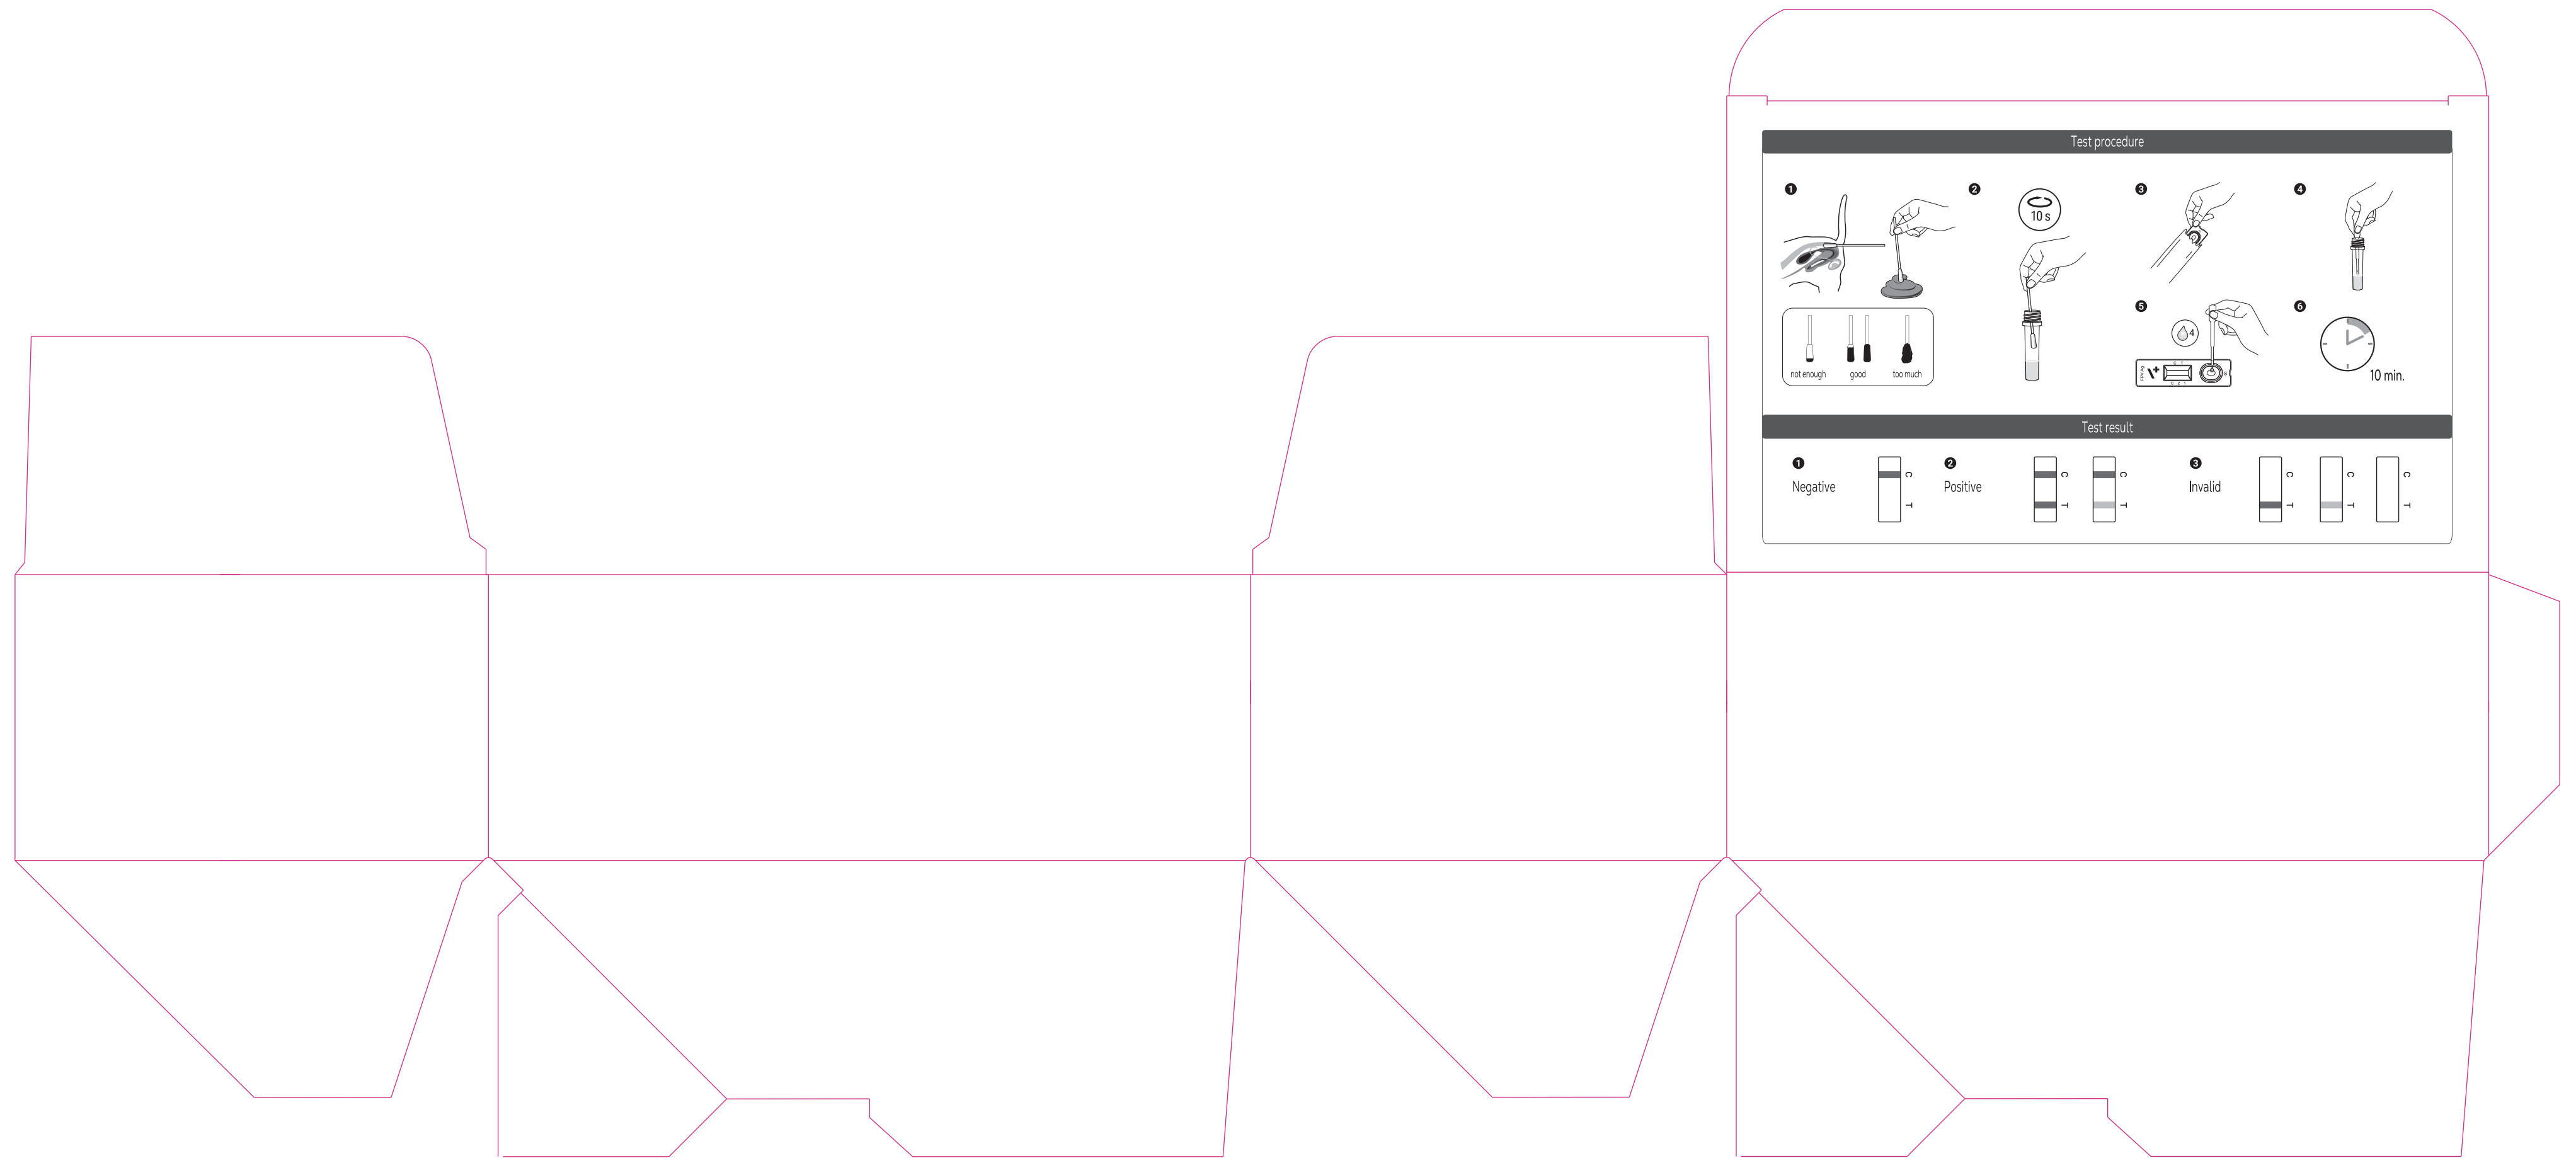
Do not reuse

Expiration date






**LOT**

Manufactured by:  
Vet Planet Sp. z o. o.  
ul. Brukowa 36/2  
05-092 Lomianki, Poland







**Test procedure**

1.  2.  3.  4.  5. 

not enough    good    too much

**Test result**

1. **Negative**  2. **Positive**  3. **Invalid** 